User Manual

1 Transfer the liquid to the powder chamber

Open the sterile packaging.

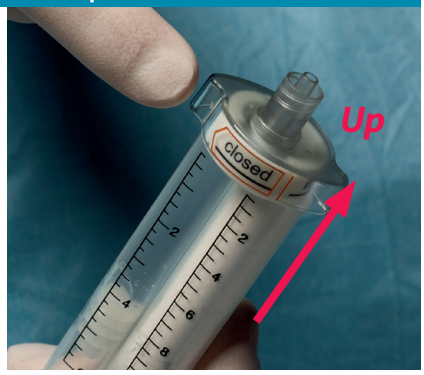

Maintain the Head UP

Rotate the collar clockwise. "transfer" appears in the red arrow

Use the plunger to push the liquid's piston...

...until all the liquid has been transferred to the powder chamber

2 The mixing phase

Keep the collar on transfer position

Mix the liquid/powder together. Be certain to reach...

...both extremities of the powder chamber.

3 Injection with the syringe

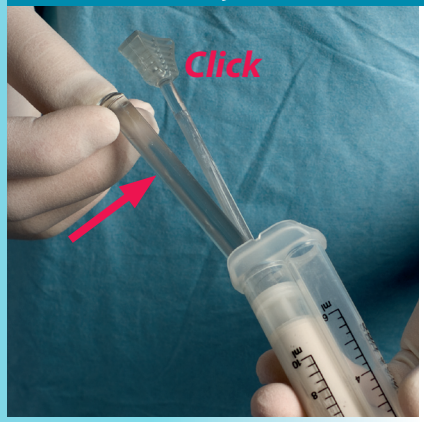

Pull the mixer to its extremity, pull the plunger from the liquid chamber. Click the plunger on the mixer.

Rotate the collar clockwise. Stop when "Inject" appears in the red arrow

If needed, connect a cannula. Push the piston and release the product.

4 Injection with the delivering gun

Keep the collar on transfer position.
Mixing time : 2 minutes

Pull and break the mixer at its base.

Connect the syringe to the delivering gun.

Rotate the collar clockwise.
Stop when "Inject" appears in the red arrow

If needed, connect a cannula.
Operate the handle in order to release the product.

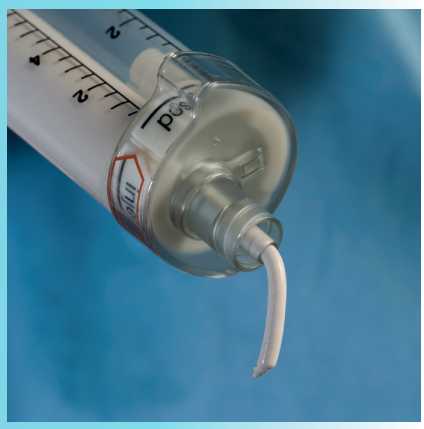

Product	Mixing time at amb. temp.	Injection time at amb. temp.	Setting time at 37°C
Graftys® HBS Hardening Bone Substitute	2 min.	15 min.	15 min.
Graftys® Quickset injectable macroporous bone substitute	2 min.	2 min.	8 min.



Graftys - *Eiffel Park- Bât. D - 415, rue Claude Nicolas Ledoux*
Pôle d'activité d'Aix en Provence - 13 854 Aix en Provence Cedex 3 - France
Phone : +00 33 (0)4 42 60 30 00 - Fax : +00 33 (0)4 42 60 30 11
www.graftys.com

UM/HBS KIT/0909A EN